


## ***AIS 2 micromanipulation system***

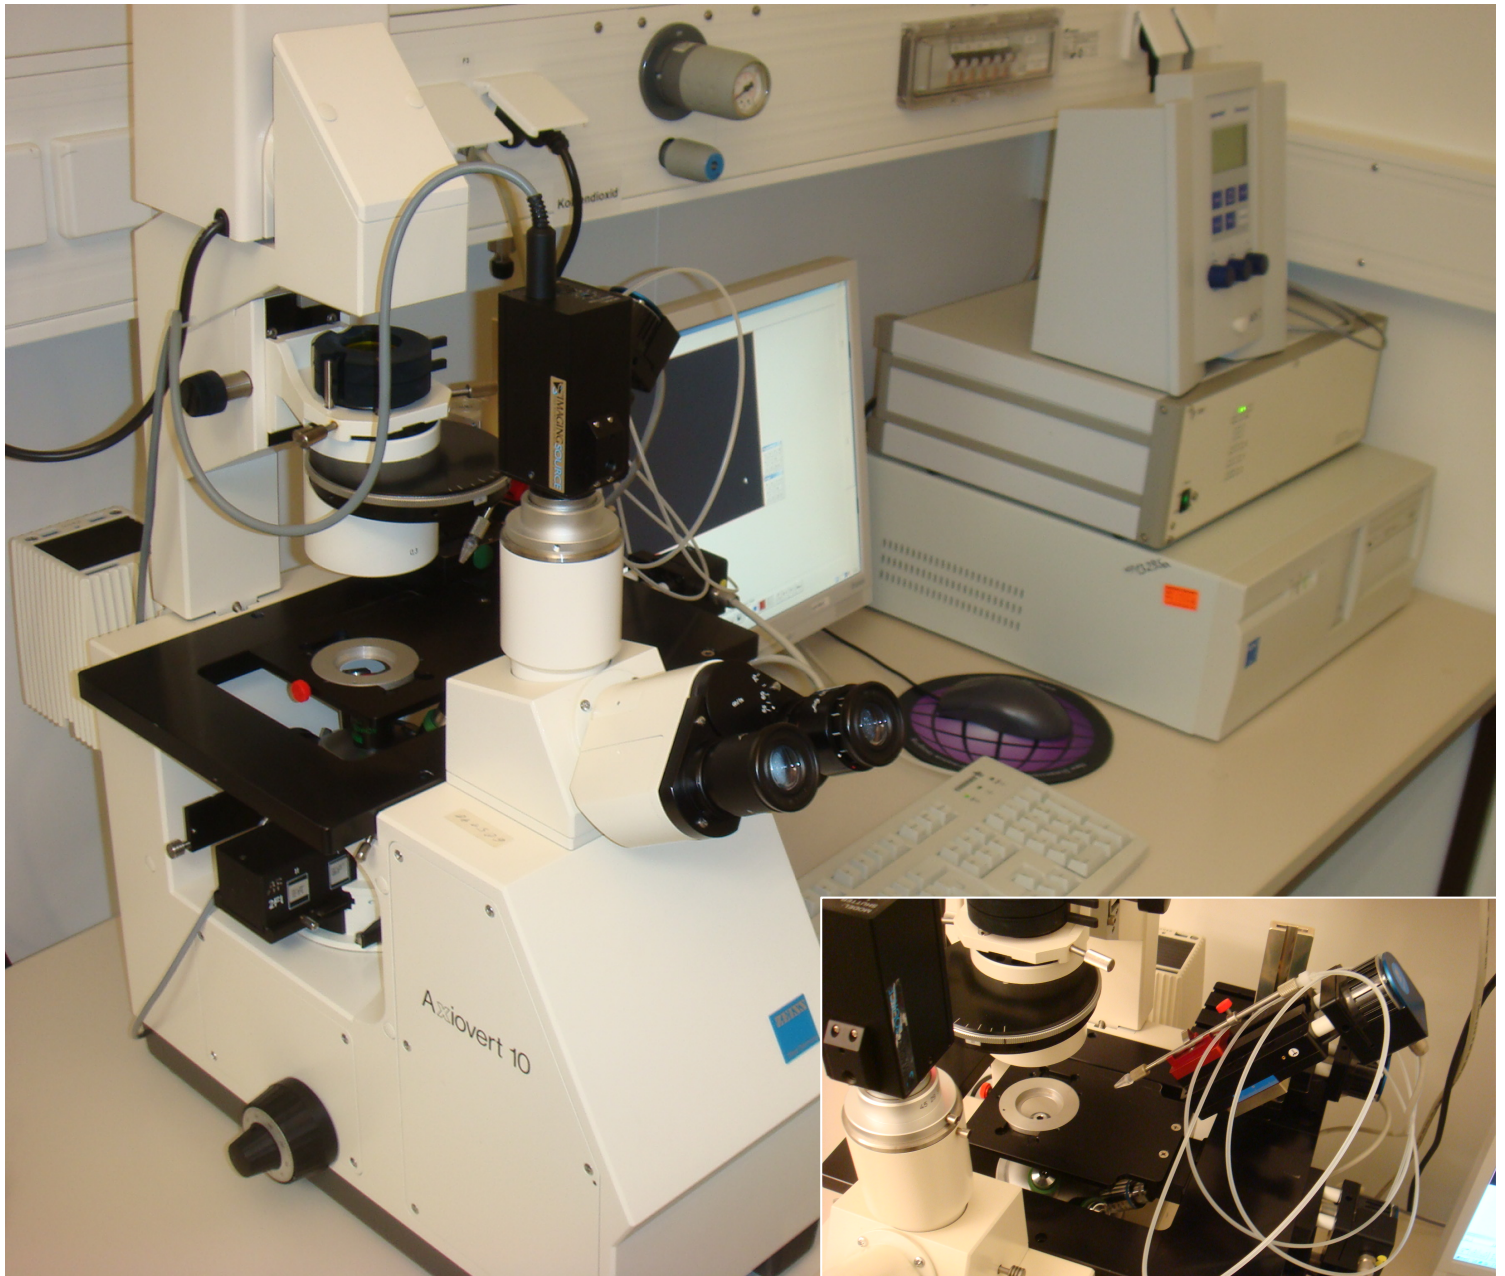

### **Short description:**

- Monochromatic camera ImagingSource DMK2002
  - Brightfield, phase contrast & fluorescence (EGFP, Cy 3.5) microscopy
  - Phase contrast at 20x & 32x magnifications
  - Luigs & Neumann injection system: x, y and axial capillary movement
  - Motorized stage: x, y and z movement
  - User interface: control program AIS 2
- Widefield microscope system for automated injection of tissue culture cells